

Data Report




기 간: 2026-06-01 00:00 ~ 2026-06-30 24:00

작성일시: 2026-07-02 17:28

간 격: 60분

작성자: 시스템관리자

저장고: CTC 초저온냉동고

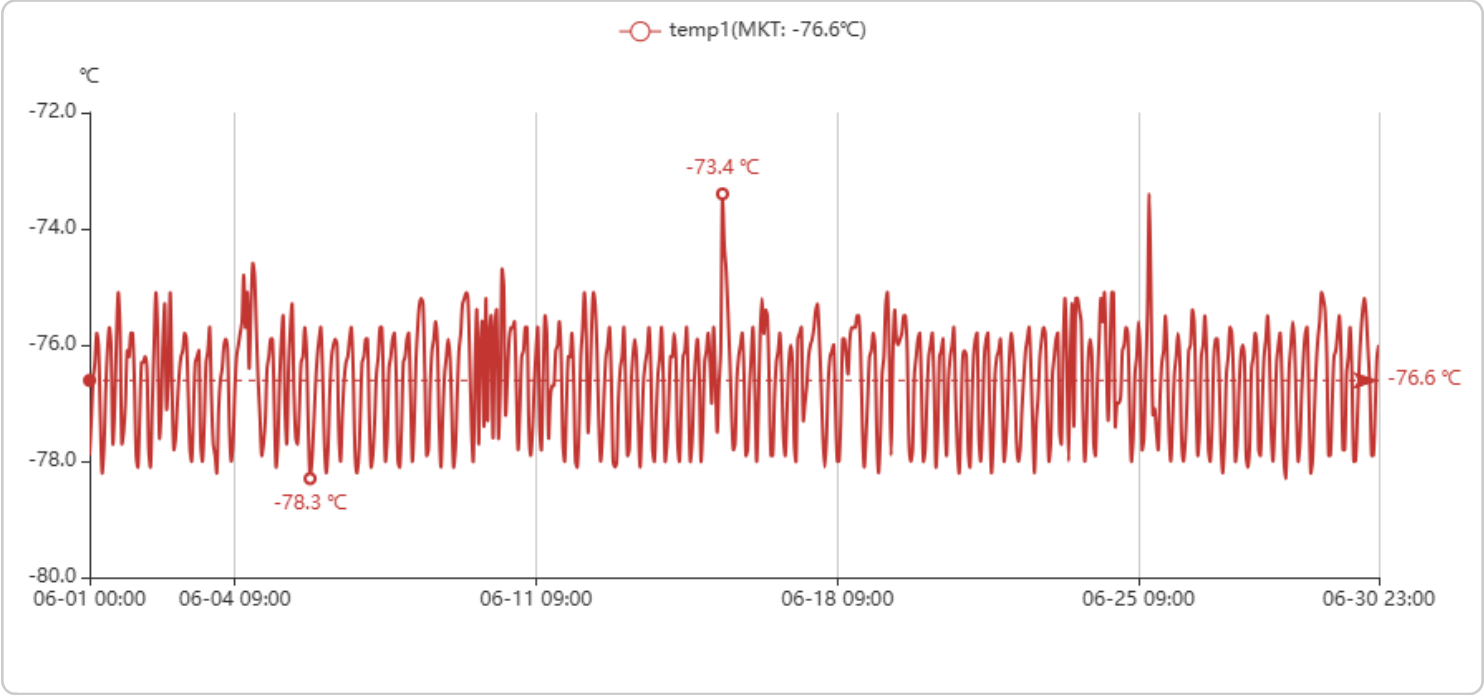

저장일시	저장고 센서 유형	측정값	하한값	상한값	전원
2026-06-30 23:00:00	temp1	-76.0 °C	-90.0	-70.0	Power
2026-06-30 22:00:00	temp1	-76.2 °C	-90.0	-70.0	Power
2026-06-30 21:00:00	temp1	-77.1 °C	-90.0	-70.0	Power
2026-06-30 20:00:00	temp1	-77.9 °C	-90.0	-70.0	Power
2026-06-30 19:00:00	temp1	-77.9 °C	-90.0	-70.0	Power
2026-06-30 18:00:00	temp1	-76.7 °C	-90.0	-70.0	Power
2026-06-30 17:00:00	temp1	-76.1 °C	-90.0	-60.0	Power
2026-06-30 16:00:00	temp1	-75.5 °C	-90.0	-60.0	Power
2026-06-30 15:00:00	temp1	-75.2 °C	-90.0	-60.0	Power
2026-06-30 14:00:00	temp1	-75.4 °C	-90.0	-60.0	Power
2026-06-30 13:00:00	temp1	-75.8 °C	-90.0	-60.0	Power
2026-06-30 12:00:00	temp1	-76.4 °C	-90.0	-60.0	Power
2026-06-30 11:00:00	temp1	-77.3 °C	-90.0	-60.0	Power